

POWER-PACKER

AN
Actuant
COMPANY


TIP SHEET 3010001259



**AIR BLEEDING
PROCEDURE MUST BE
FOLLOWED ON ALL
UNITS AFTER
SHIPPING AND PRIOR
TO INSTALLATION.
FAILURE TO DO SO
WILL RESULT IN
IMPROPER
PERFORMANCE
CHARACTERISTICS.**

SCSA – AIR BLEEDING PROCEDURE

ALL SELF CONTAINED STRETCHER ACTUATORS MUST BE AIR BLED AFTER SHIPPING AND BEFORE INSTALLATION BY THE FOLLOWING PROCEDURE TO INSURE PROPER PERFORMANCE.

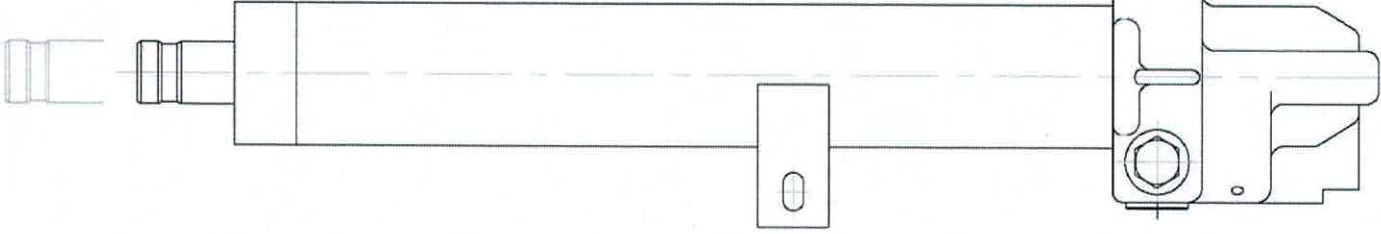

AIR BLEED PROCEDURE

- 1.) ORIENT UNIT VERTICALLY WITH ROD END UP.
- 2.) OPERATE UNIT TO FULL EXTEND USING PUMP PLUNGER.
- 3.) PUMP UNIT 3-4 MORE TIMES AFTER FULL EXTEND.
- 4.) DEPRESS RETRACT PLUNGER AND APPLY LOAD TO ROD TO RETRACT UNIT COMPLETELY.
- 5.) REPEAT FOR 3 CONSECUTIVE CYCLES.
- 6.) UNIT MAY NOW BE INSTALLED ON STRETCHER.

NOTE:

THIS PROCEDURE DOES NOT APPLY IF UNITS ARE RECEIVED FROM MANUFACTURER IN PRODUCTION PACKAGING WITH VERTICAL ORIENTATION MAINTAINED.

POWER-PACKER
516 Hillcrest Drive.
Westfield, WI 53964
800/745-4142
www.powerpacker.com

3010001259
REV. 0A
07/19/07